Print on Plain White Paper (Part No. 122919)

MIDMARK®

Installation Instructions

9A198001 ROUND HEADREST
9A199001 SPECIAL PROCEDURES HEADREST

KIT COMPONENTS

Part Number	Description	Qty.
9A198001	Round Headrest	1
or		
9A199001	Special Procedures Headrest	1
003-0940-00	Installation Instructions	1

INTRODUCTION

To provide access to a patient's head during examinations / procedures.

NOTE

The 9A198001 and 9A199001 will not adapt to the 9A221001 One Arm Wrist Rest Assembly.

REQUIRED TOOLS

None

INSTALLATION

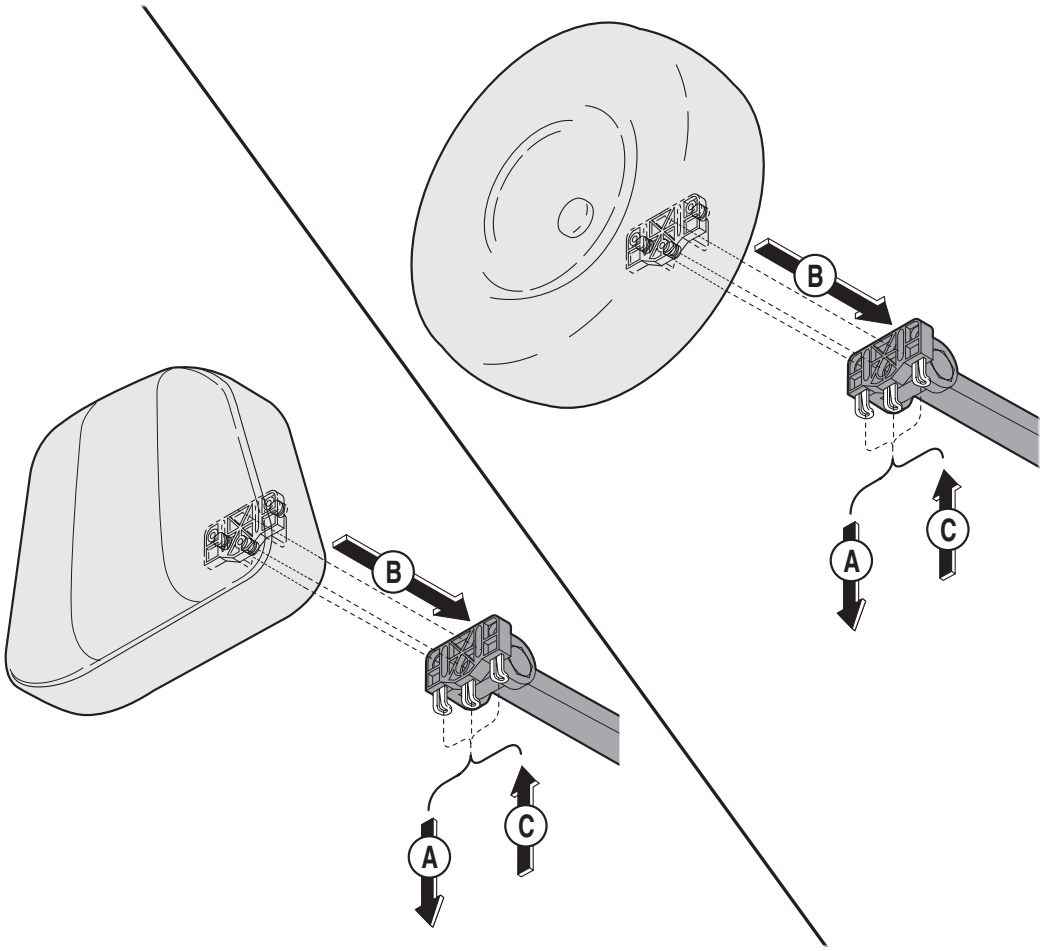

MA442000

A. Pull downward on slide bars and remove existing headrest.
B. Place desired headrest on pivot mount.
C. Push upward on slide bars to lock headrest to pivot mount.

MIDMARK®

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

003-0940-00 Rev. B (4/01)

© Midmark Corporation - 2001